

COMITATO NAZIONALE PER L'ENERGIA NUCLEARE
Laboratori Nazionali di Frascati

LNF-62/73

F. Pandarese, F. Villa: TUNNEL DIODE FAST DISCRIMINATOR CIRCUIT.

Nota interna: n° 158
5 Settembre 1962

Laboratori Nazionali di Frascati del C.N.E.N.
Servizio Documentazione

LNF-62/73

Nota interna: n° 158
5 Settembre 1962

F. Pandarese^(x), F. Villa⁽⁺⁾: TUNNEL DIODE FAST DISCRIMINATOR CIRCUIT.

SUMMARY

A fast integral discriminator, employing tunnel diodes arranged in a bridge-like configuration, is examined.

Diagrams and characteristics of the circuit are given.

The discriminator has been designed to operate in series with a 125 ohm cable, to allow the driving pulse to be used for other purposes. The mismatching introduced using the circuit and components of fig. 1 is less than 5%.

The pulse to be discriminated travels along the cable in the direction shown by the arrow. If its amplitude is such as to let a current greater than I_p to flow in each arm of the bridge, tunnel diodes TD2 and TD3 switch into their high impedance region and an output pulse of .4 v appears at the

(x) - Laboratori Nazionali di Frascati del C.N.E.N.

(+) - Sezione di Roma dell'I.N.F.N. - Scuola di Perfezionamento Sezione di Roma.

secondary windings of the transformer, while the driving pulse, reduced in amplitude keeps on travelling to the right. The reduction, when the discriminator switches on, is .4 v, independently of threshold setting; if it is not switched on the reduction is less than 5% of trigger pulse amplitude. In the above mentioned case only tunnel diodes TD2 and TD3 have been effective, whereas TD1 and TD4 behave like resistors. Should the polarity or the direction of propagation of driving pulse be reversed, then TD1 and TD4 will be effective and the output of the transformer will be of opposite polarity. 3.5 ohm resistors may be used instead of TD2 and 3, or TD1 and 4, when reversing the direction of propagation of driving pulse is a feature not needed. The resistors used are shown in figure 7.

The advantages of using bridge-like arrangements are well known⁽¹⁾. Using two tunnel diodes instead of one for instance TD2 and TD3), doubles the output pulse, bringing it to a level (0.4V) which is more suitable for driving directly subsequent transistor circuitry^(x). Using the transformer in the output instead of the input⁽²⁾ makes the recovery time for pulses below threshold independent of the transformer recovery time and practically negligible; another very useful consequence is the complete independence (within measurement accuracy, 1 ns) of input to output pulse delay, from input overvoltage.

The transformer turns ratio may be changed within a factor 3 - to achieve a compromise, between output pulse le-

(x) - Should be pointed out that the discriminator cited in ref. (2) was intended for use as a timer based on zero crossing of photomultiplier pulses.

vel and time definition (including recovery time). Figs. 2 and 6 show the wave forms obtained with 1:3 and 1:1 turns transformer, respectively. Note that in both cases the difference between peak currents of the two switching tunnel diodes is 5%.

Using the 1:3 transformer, the recovery time after a single pulse just above threshold (defined at 5% overdrive for a second pulse to give an output) is 20 ns. For this measurement both the trigger pulses were 5 ns long. The variation of the output pulse height vs input overdrive is shown in fig. 4. Such large variation does not effect the use of the device as a trigger with very fast input characteristics. The threshold variation as a function of polarization current is shown in fig. 5. Threshold variation vs pulse lenght is shown in fig. 5.

Using the 1:1 transformer, the recovery time becomes somewhat greater, depending on bias and load conditions. The output pulse height, however, increases only by 20% for an input over drive variation between 1 and 10.

The performance of the device has been tested with a burst generator, giving 100 s bursts of 15 ns pulses spaced 70 ns. The threshold for the burst was found to be 20% higher than the threshold for a single pulse, this being obviously due to the effect of the inductive output coupling.

A burst below threshold, however, was found practically ineffective on the single pulse threshold, as expected.

Another mounting arrangement, using commercial resistors instead of germanium resistors, has been experimented. The only noticeable change in performance, probably due to parasitic inductance, was the minimum pulse length, 8 ns, for which the threshold is kepted constant.

Acknowledgments


The authors wish to express their thanks to Prof. E. Gatti and Prof. L. Mezzetti for advice and useful suggestions, and to Prof. I.F. Quercia for constant encouragement.

References

- (1) H. Ur, "Tunnel diode High-Energy Circuits", Proc. Intern. Conference on Instrumentation for High-Energy Physics, Berkeley Sept. 1960, pg. 45.
- (2) Q. Kerns, A. Bjerke, T. Nunamaker, "Tunnel diode discriminator", Proc. Intern. Conference on Instrumentation for High-Energy Physics, Berkeley Sept. 1960, pg. 62.

TUNNEL DIODE DISCRIMINATOR CIRCUIT

FIG. 1

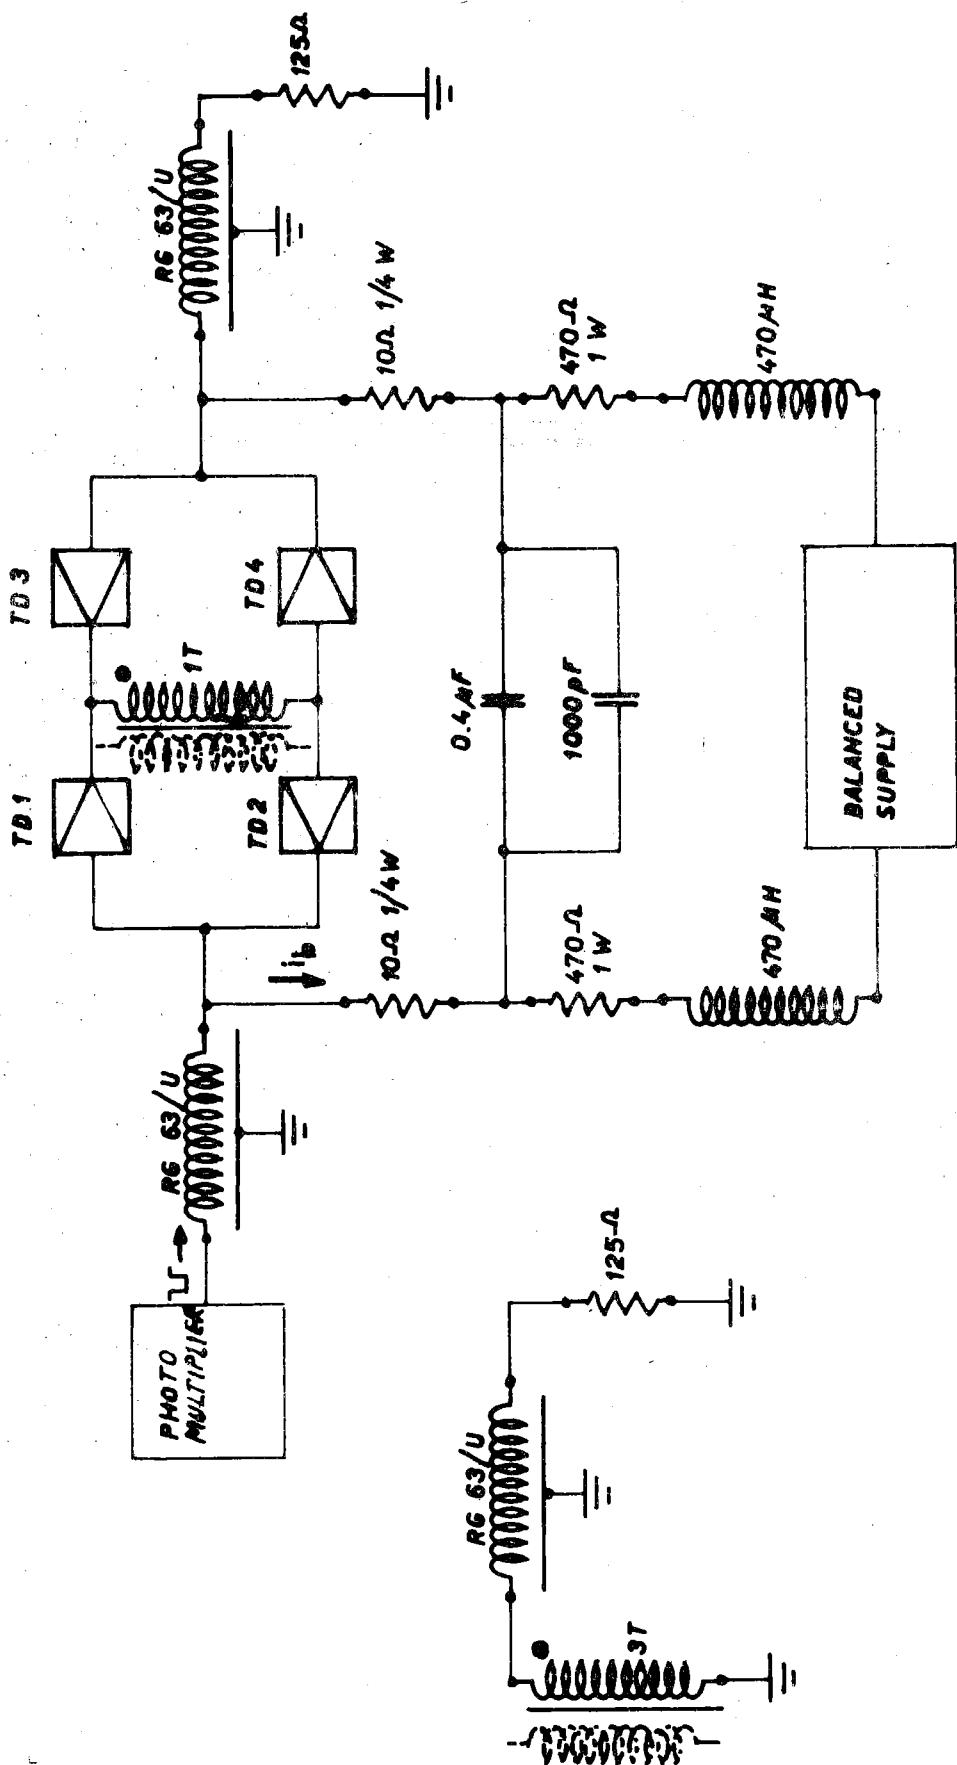

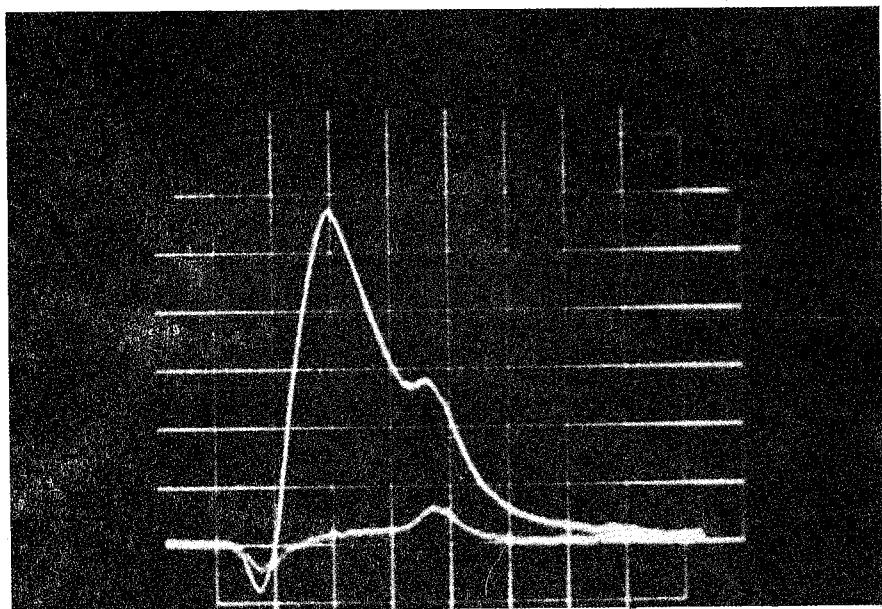


FIG. 2 - OUTPUT PULSE FOR PULSE SLIGHTLY BELOW
AND ABOVE THRESHOLD: vert. 1 v/cm, hor. 4 ns/cm

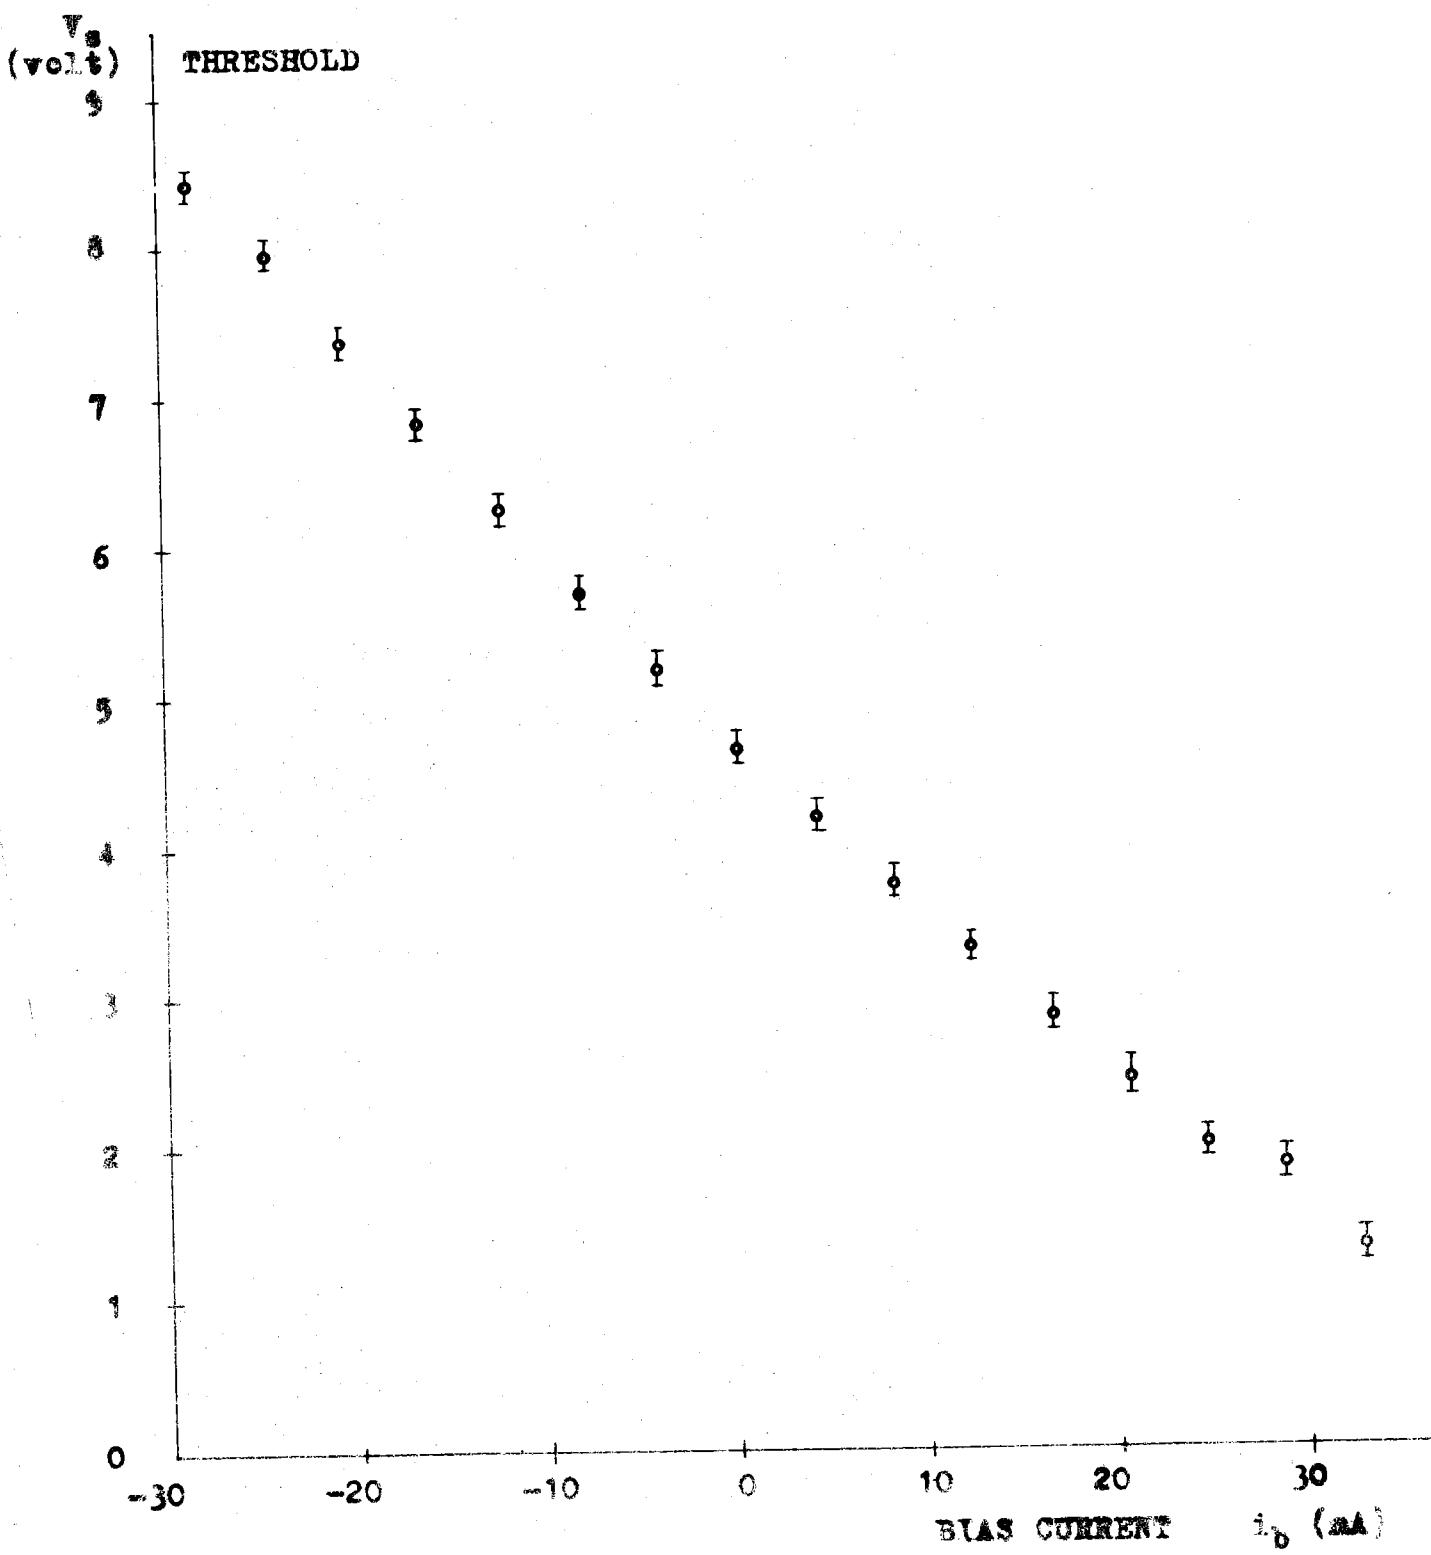
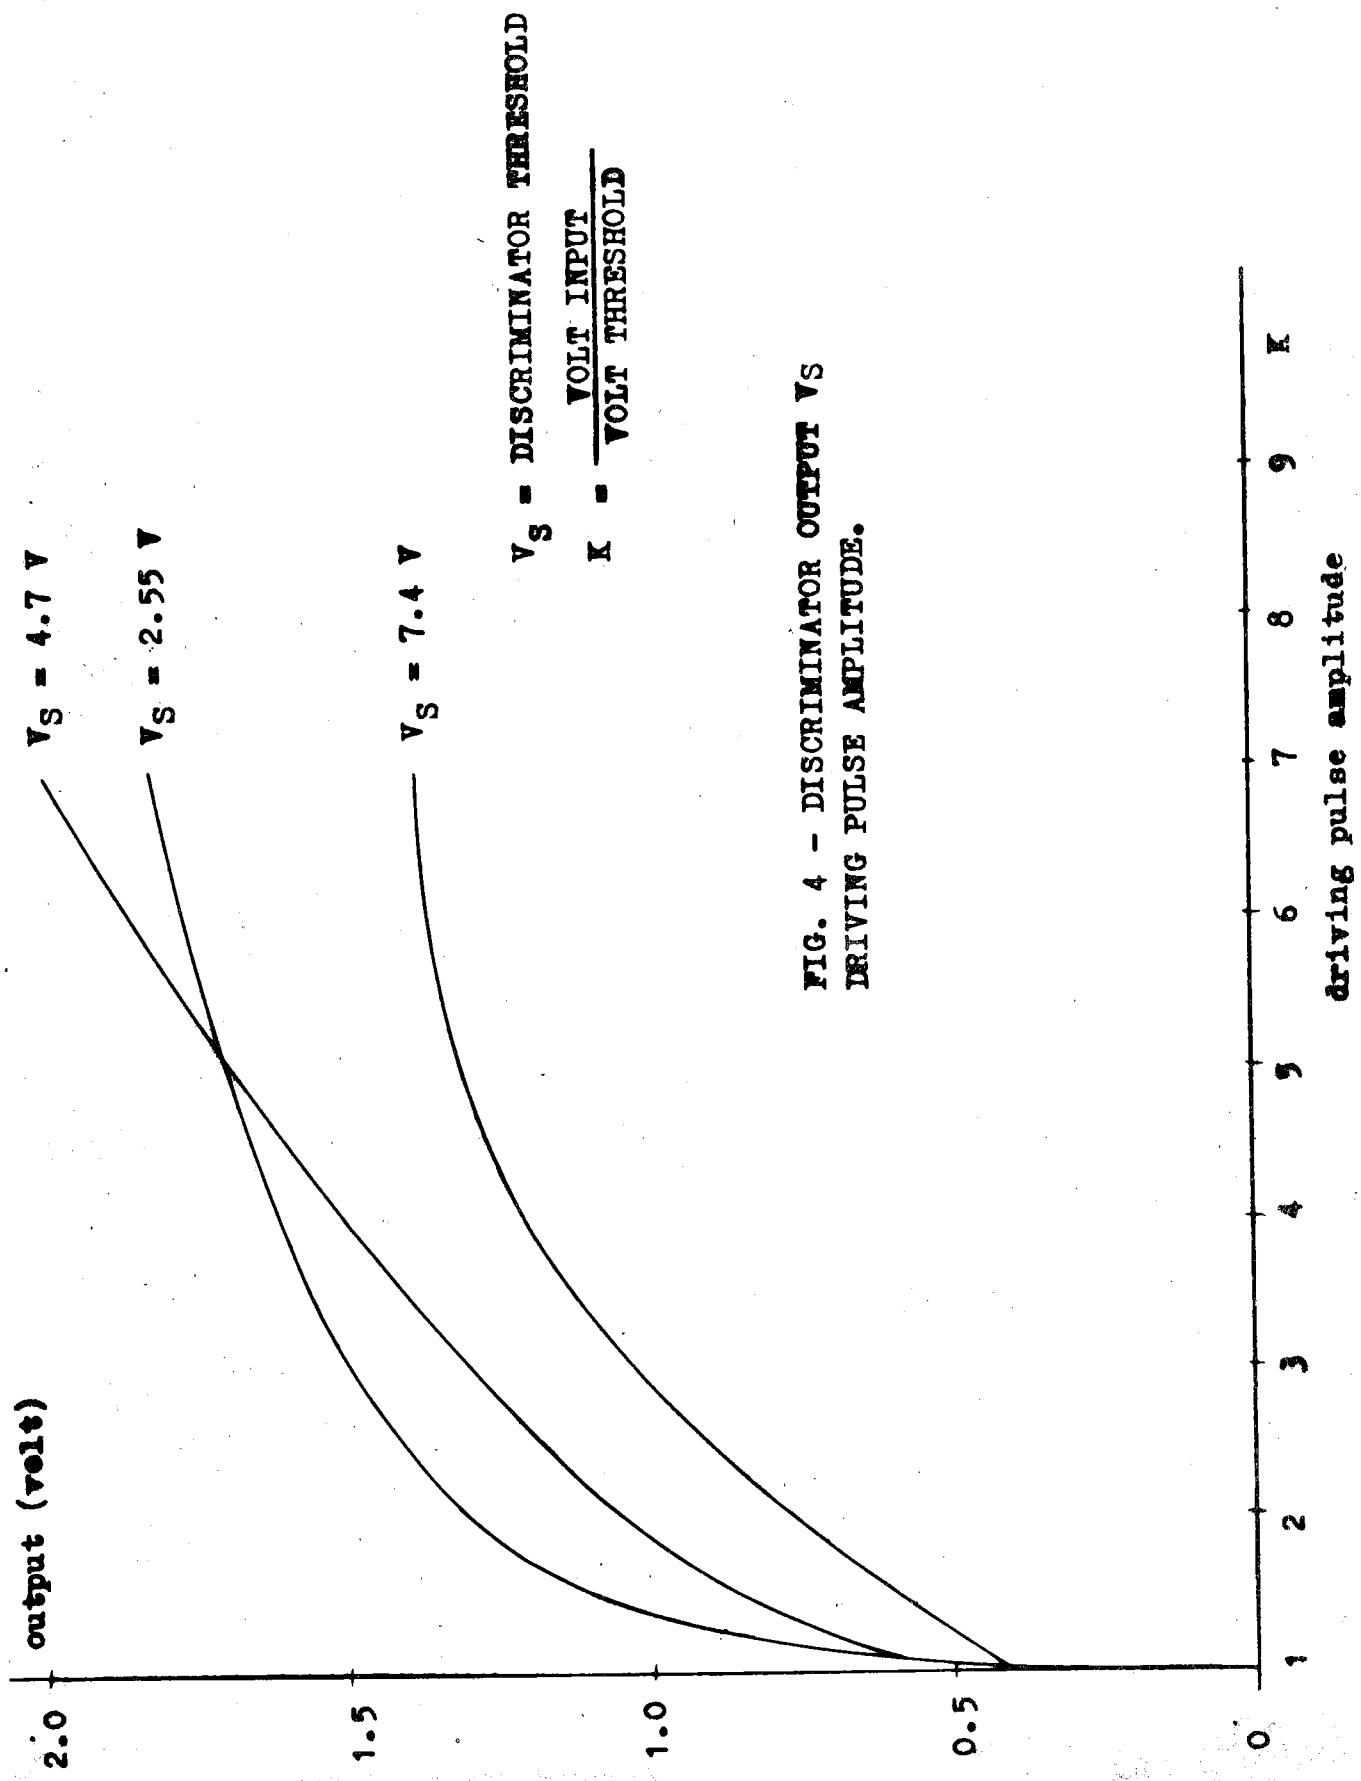


FIG. 3 - DISCRIMINATOR THRESHOLD vs BIAS CURRENT.



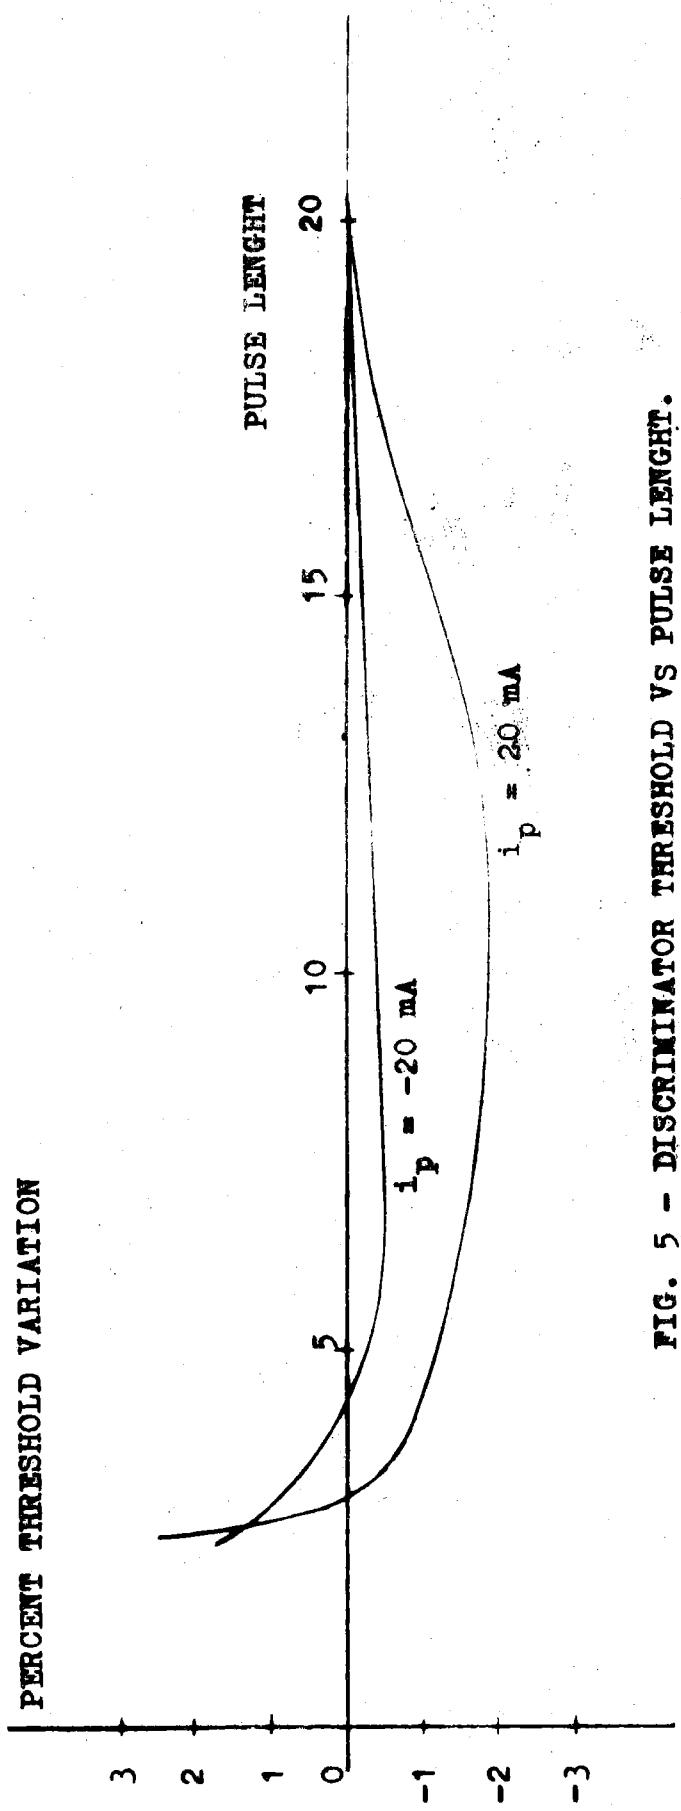


FIG. 5 - DISCRIMINATOR THRESHOLD VS PULSE LENGTH.
ERROR ON EXPERIMENTAL POINTS IS 0.5%.

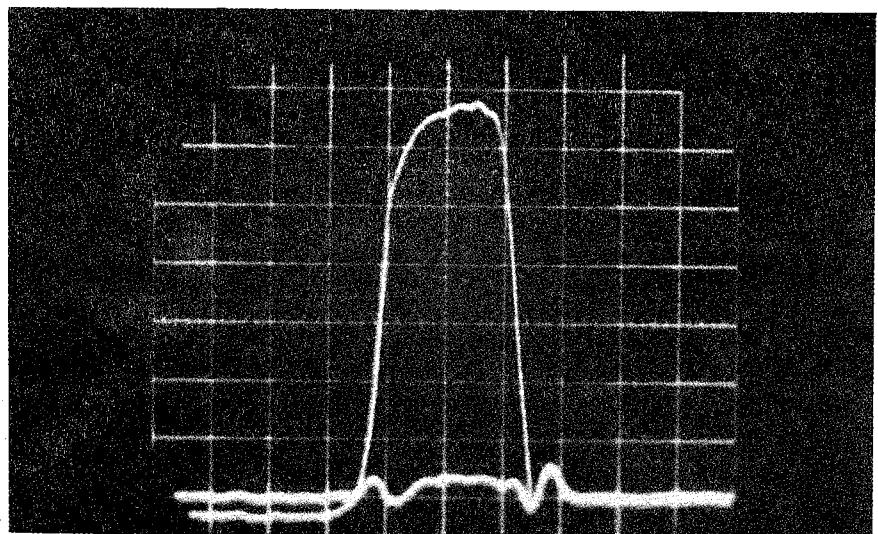


FIG. 6 - OUTPUT PULSE FOR A IT/IT TRANSFORMER:
vert. 0.05 v/cm, hor. 4 ns/cm

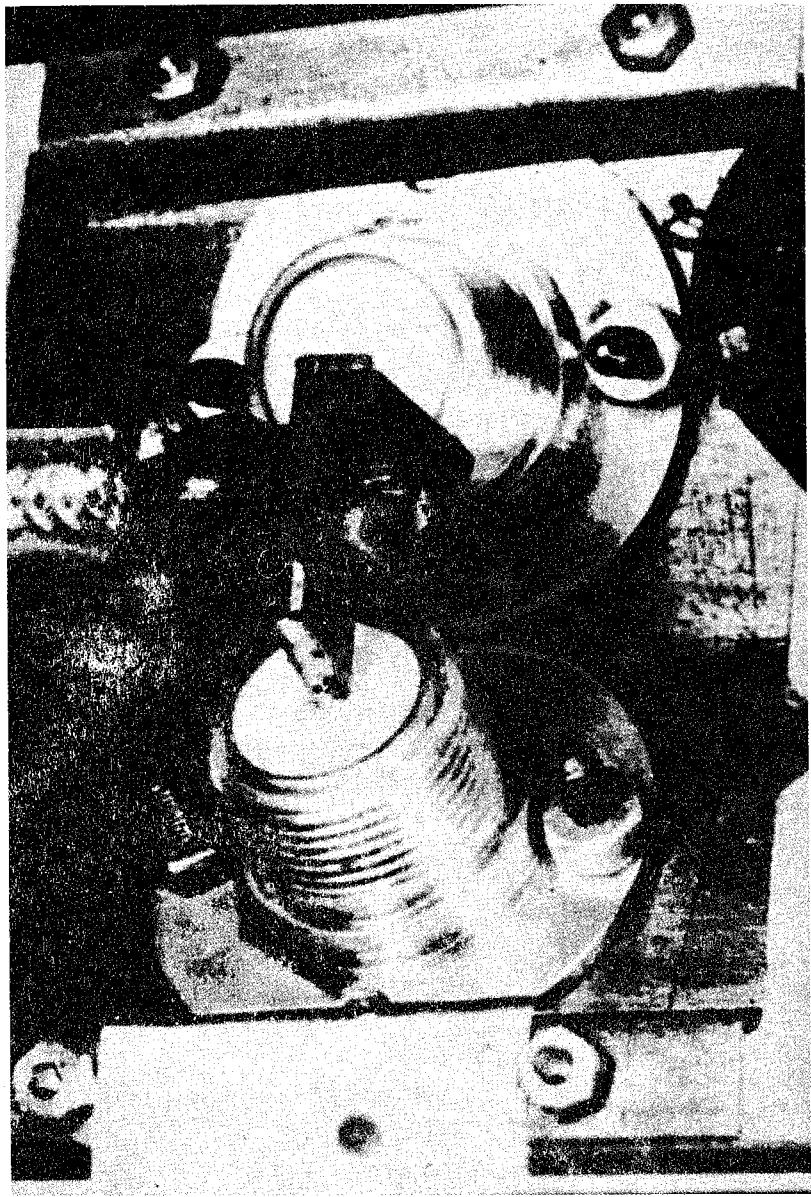


FIG. 7 - COMPONENT LAY OUT SHOWN IN BOTTOM VIEW
OF CHASSIS WITH POLARIZATION CIRCUIT REMOVED.
AT RIGHT p-TYPE GERMANIUM 3.5 OHM RESISTORS,
WITH CONTACT SURFACES ELECTROLITICALLY GOLD -
PLATED.