

LNF-08/18(P)
October 26, 2008

JINR E2-97-141
hep-th/9707240

**ELEMENTAL MAPPING AND MICRO-IMAGING BY X-RAY
CAPILLARY OPTICS**

Dariusz Hampai,^{1,2,3,*} Sultan B. Dabagov,^{2,4} Giorgio Cappuccio,²
Antonio Longoni,⁵ Tommaso Frizzi,⁵ Giannantonio Cibin,⁶
Valeria Guglielmotti³ and M. Sala⁷

¹*INOA-CNR, L.go E. Fermi, 6, I-50125 Firenze, Italy*

²*INFN-LNF, Via E. Fermi, 44, I-00040 Frascati (RM), Italy*

³*MINASlab, Dipartimento di Scienze e Tecnologie Chimiche,
Università di Roma "Tor Vergata"*

⁴*RAS - P.N. Lebedev Physical Institute, Leninsky pr. 53, 119991 Moscow, Russia*

⁵*Politecnico di Milano, Dipartimento di Elettronica e Informazione,
Via Golgi, 40, 20133, Milan, Italy*

⁶*Diamond Light Source Ltd., Chilton, Didcot OX11 0DE, UK*

⁷*Dip. di Scienze della Terra A. Desio, Univ. di Milano, Italy*

*Corresponding author: dariusz.hampai@lnf.infn.it

Abstract

Recently, many experiments have highlighted the advantage of using polycapillary optics for x-ray fluorescence studies. We have developed a special confocal scheme for micro x-ray fluorescence (μ XRF) measurements, which enables us to obtain not only elemental mapping of the sample but also simultaneously its own x-ray imaging. We have designed the prototype of a compact x-ray spectrometer characterized by a spatial resolution of less than 100 μ m for fluorescence and less than 10 μ m for imaging. A couple of polycapillary lenses in a confocal configuration together with a silicon drift detector (SDD) allow elemental studies of extended samples (\sim 3 mm) to be performed while, a charge-coupled device (CCD) camera makes it possible to record an image of the same samples with a 6 μ m spatial resolution, which is limited only by the pixel size of the camera. By inserting a compound refractive lens (CRL) between the sample and the CCD camera, we hope to develop an x-ray microscope for more enlarged images of the samples under test.

OCIS codes 340.7440, 340.7460, 180.2520, 170.1790, 180.1790, 040.6040

Accepted to Optics Letter at 10th of October 2008

1 Introduction

Nondestructive analysis of archaeological artifacts by micro x-ray fluorescence spectrometry (μ XRF) is a promising multi-elemental technique that has rapidly developed during the last few years [1,2]. With the exception of synchrotron radiation, which is a suitable probe for micro spots, it is often challenging to perform table-top μ XRF analysis. However, the difficulty of producing and focusing small-size x-ray beams can limit the feasibility of this type of analysis.

The polycapillary lenses designed for x-ray beam focusing now offer alternative laboratory solutions[3–7]. The combination of a polycapillary lens and a fine focus x-ray tube (with a source spot diameter less than $50\ \mu\text{m}$) can provide the high-intensity radiation flux necessary to perform elemental analysis. Compared to a pinhole or to a monocapillary [8], an optimized “x-ray source-optics system” can result in a radiation density gain of more than three orders of magnitude (by radiation density gain we mean the ratio of x-ray intensity at the focal spot with and without the optics) [3]. In such a way, due to the rather high-intensity irradiation on a limited space, non-destructive μ XRF analysis becomes possible. The most advanced way to get this result is to use a confocal configuration with two x-ray polycapillary lenses. One lens is responsible for the fluorescence excitation on the sample; the other allows detection of the secondary emission from the sample (see for instance [4]). With a μ XRF instrument based on x-ray micro-focusing by two polycapillary lenses, 3D elemental mapping can be obtained [9]. Our final aim is to design a portable x-ray microscope to provide simultaneously on-site μ XRF mapping analysis. To focus the x-ray beam we are actually using polycapillary optics, but in the near future we plan to use a polycapillary lens as a concentrator and a compound refractive lens (CRL) for the magnification [10]. Since this kind of spectroscopy is non-destructive, we believe it could be useful in the analysis and interpretation of archaeological artefacts and remains.

2 Experimental Setup and First Results

An experimental setup with a cabinet and an optical table was designed and developed specifically for R&D of x-ray optical systems at the Laboratori Nazionali di Frascati (LNF) [11]. The radiation source is a 50 W Cu x-ray tube (Oxford Apogee 5000) with a source spot size of about $50\ \mu\text{m}$. There are four different detector units available: a scintillator with an effective working area of ~ 1 square in.; two Photonic Science charged-coupled device (CCD) cameras with the software package “Image Pro” for x-ray rough/fine imaging; a silicon drift detector (SDD) with a $5\ \text{mm}^2$ working area[12,13]. The

first ccd camera (FDI 1.61:1) has a sensitive area of 4x3 mm with a 3.5x3.5 μm resolution; the second (FDI 1:1.61), an active area of 14.4x10.8 mm with a resolution of 10.4x10.4 μm .

The first microscope designed recently at LNF [14,15] was made with an x-ray source, a CCD detector, and a semi-lens. By choosing a semi-lens we hoped to get a very small blurring effect because of the fairly small radiation divergence behind the optics (without taking into account diffraction effects on the sample edges, i.e., far from a wave zone, as well as multiple scattering radiation in matter). To evaluate the highest resolution available, we used a sample of standard mesh: Au 1000 with a hole width of 19 μm and bar width of 6 μm (Fig. 1).

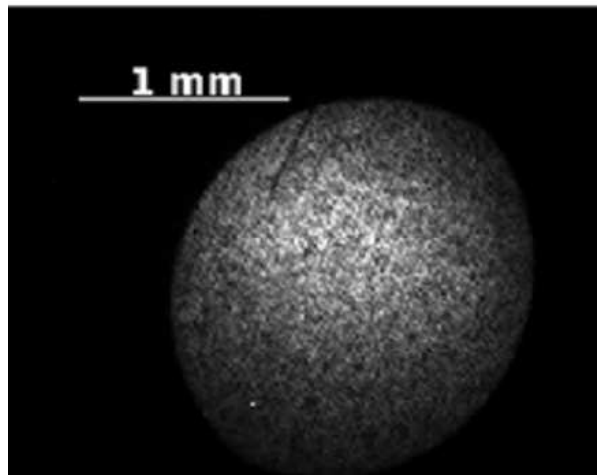


Figure 1: High resolution image of a gold mesh 1000 recorded by the detector (FDI 1.61:1) placed at a distance of ~ 44 cm from the sample.

As an additional option, a second polycapillary lens inserted between the sample and the detector made it possible to implement the μXRF unit with a prototype of an x-ray projection microscope. Polycapillary optics (Unisantis S.A.) with a full lens shape were used to focus the divergent beam from the x-ray Cu tube onto the sample. Another lens in “confocal geometry” allowed detection of the sample x-ray fluorescence with a nominal focal spot size of less than 100x100 μm . In recent years a lot of reported work has shown the advantages of this optical configuration to perform simultaneously micro-fluorescence mapping and imaging[4,6,5]. To obtain the confocal configuration we used two full lenses, chosen so as to have the smallest focal spot and the highest transmission. The first lens provides a focal spot of ~ 90 μm and 50% transmission; the second has a spot of ~ 100 μm and 42% transmission. The prototype scheme is shown in Fig. 2.

Fig. 3 reports our first μXRF spectrum collected in 60 s on a Neolithic human

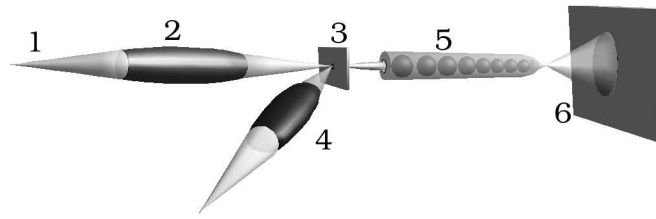


Figure 2: Final prototype layout for μ XRF and imaging: 1 - the X-ray source; 2 and 4 - the 1st and 2nd polycapillary optical elements, respectively; 3 - the sample; 5 - a Compound Refractive Lens (CRL) for Imaging; 6 - CCD detector.

bone sample in powder form where all main elements are well resolved with an excellent collected intensity and good signal to noise ratio (Cf. [16]).

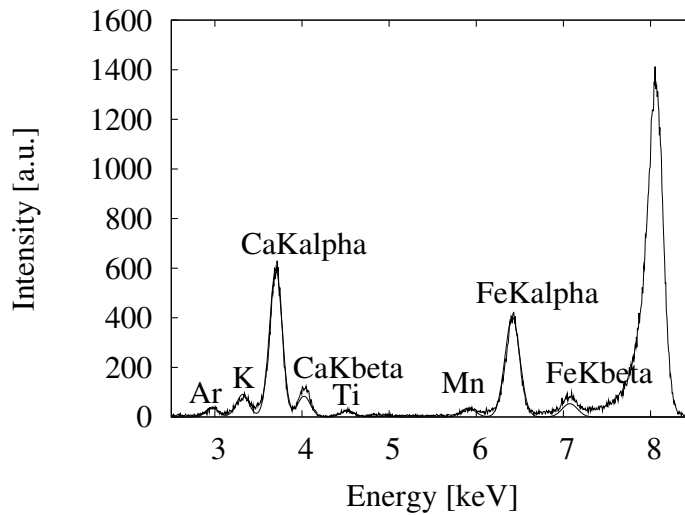


Figure 3: μ XRF spectrum of a neolithic human bone powder sample obtained in confocal configuration.

A real mapping of μ XRF spectroscopy was obtained on standard sample of ferric oxide (Fe_2O_3) [9]. The standard monophasic minerals of Fe_2O_3 was prepared in a 1000 class clean room at DISAT, University of Milano - Bicocca. So as not to overlap two close measurements, we made a scan, by a remote system, of 4x4 mm of the region with a step movement of 200x200 μm . Fig. 4 shows the image result: red represents iron (in intensity scale of gray); the white bright pixels are manganese (contamination is probably present so we are designing a glow box for performing measurements in a helium atmosphere).

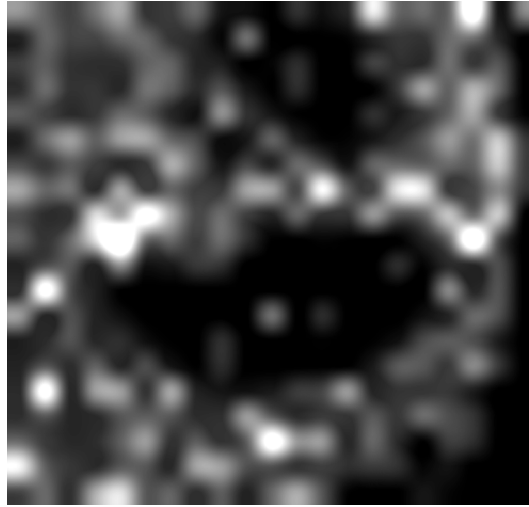


Figure 4: μ XRF mapping spectrum Ferrum Oxide sample, deposited on a silicon wafer. The gray pixels represents iron (in a scale of gray), while the white bright spots are manganese trace. The measured area is 4x4 mm with a step sized of 200x200 μ m.

3 Conclusions

We have described a new prototype for μ XRF analysis. We have shown that a confocal optical scheme used with a low-power (50 W) conventional tube and high-resolution SDD detector becomes a powerful instrument for x-ray fluorescence measurements of micro-size spot. Polycapillary lenses in a “confocal configuration” deliver with a micro-size spot a high photon flux on a sample, so they are ideal candidates for overcoming some of the main problems of laboratory x-ray instruments, including signal-to-noise ratio, resolution, mapping, and portability.

We have shown the first results both for x-ray imaging and for XRF spectroscopy. With regard to imaging, the use of a polycapillary semi-lens helps us get a spatial resolution of about 6 μ m. To decrease the x-ray spot dimensions, we would like to substitute the present polycapillary lenses with the latest generation lenses since they provide a focal spot of a few microns in diameter. To increase the x-ray microscopy resolution, we are planning to combine a full polycapillary lens with a compound refractive lens.

References

- [1] “ICXOM 2005”, Frascati, Italy, September 25-30, 2005; Spect. Acta B Vol. 62, (6-7), 515-720 (2007)

- [2] "ICXOM 2007", Kyoto, Japan, September 16-21, 2007; submitted to *Spect. Acta B* (2007).
- [3] S.B. Dabagov, "Channeling in Neutron Particles in micro- and nanocapillaries", *Physics Uspekhi* **46** (10), 1053 - 1075 (2003).
- [4] N. Zoeger, C. Strelis, P. Wobrauschek, C. Jokubonis, G. Pepponi, P. Roschger, J. Hoffstaetter, A. Berzlanovich, D. Wegrzynek, E. Chinea-Cano, A. Markovicz, R. Simon and G. Falkenberg, "Determination of the elemental distribution in human joint bones by SR micro XRF", *X-Ray Spect.* **37** (1), 3-11 (2008).
- [5] K. Nakano and K. Tsuji, "Development and application of confocal 3D-micro-XRF spectrometer", ICXOM 2007, submitted to *Spectrochimica Acta B* (2007).
- [6] M. Bielewski, J. Himbert, M. Betti and R. Simon, "Application of the confocal -XRF for 3D analysis of elements distribution in hot environmental particles", ICXOM 2007, submitted to *Spectrochimica Acta B* (2007).
- [7] Lin Xiao Yan, Wang Zhi Hong, Chu Xue Lian, Sun Tian Xi and Ding Xun Liang, "Investigation of a Tabletop Confocal Micro X-Ray Fluorescence Setup", *Chin. Phys. Lett.* **24** (12), 3368-3370 (2007).
- [8] W. Chang, J. Kerner and E. Franco, "Analytical Micro X-ray Fluorescence Spectrometer", *Adv. in X-Ray Analysis*, Vol **44**, 325 - 328 (2001).
- [9] D. Hampai, S.B. Dabagov, G. Cappuccio, A. Longoni, T. Frizzi, G. Cibin, V. Guglielmotti, M. Sala and V. Sessa, "X-ray microfocusing by polycapillary optics", *Proc. of Spie Vol.* **7707**, 70770U (2008).
- [10] G. Cappuccio, S.B. Dabagov, D. Hampai, Yu.I. Dudchik and F.F. Komarov, "A spherical compound refractive lens to control x-ray beams ", *Proc. Spie Vol.* **6634**, 66341M (2007).
- [11] G. Cappuccio, G. Cibin, S.B. Dabagov, A. Esposito, D. Hampai, A. Marcelli, V. Sessa, C. Veroli, M.A. Kumakhov and R.V. Fedorchuk, *LNF Activity Report 2004*, 181 - 182 (2004). www.lnf.infn.it/rapatt
- [12] R. Alberti, C. Fiorini, C. Guazzoni, T. Klatka and A. Longoni, "Elemental mapping by means of an ultra-fast XRF spectrometer based of a novel high performance monolithic array of silicon detectors", *Nucl. Instr. Meth.* **B580** (2), 1004-1007 (2007).

- [13] R. Hartmann, D. Hauff, P. Lechner, R. Richter, L. Struder, J. Kemmer, S. Krisch, F. Scholze and G. Ulm, “Low energy response of silicon pn-junction detector”, Nucl. Instr. Meth. **A377**, 346 - 351 (1996).
- [14] D. Hampai, S.B. Dabagov, G. Cappuccio and G. Cibir, “X-ray propagation through hollow channel: PolyCAD a ray tracing code”, Nucl. Instr. Meth. **B244**, 481-488 (2006).
- [15] D. Hampai, S.B. Dabagov, G. Cappuccio, G. Cibir and V. Sessa, “Modeling of X-ray transport through polycapillary optics”, Nucl. Instr. Meth. **A589**, 85-89 (2007).
- [16] S. Joschek, B. Nies, R. Krotz and A. Gopferich, “Chemical and physicochemical characterization of porous hydroxyapatite ceramics made of natural bone”, Biom. **21**, 1645 - 1658 (2000).